


INNOVA (BMRHWINV) – STAND

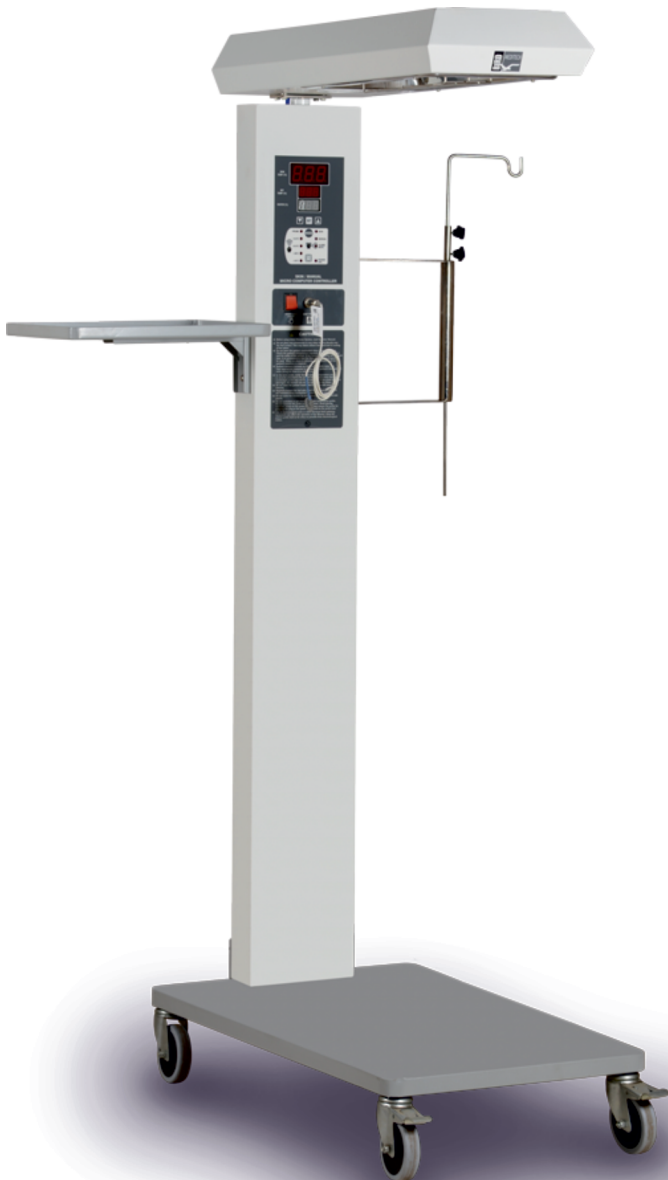

Components

Micro Computer Temperature Controller

- PID (proportionate integrated derivative) based micro processor technology assures accurate maintenance of set temperature with internal accuracy of 0.01°C
- User friendly on-board temperature calibration with feather touch keys
- User friendly feather touch control
- Key-pad lock facility to avoid accidental changes of any set parameters
- Safety alarm with high temperature cutoff
- Watch Dog facility Auto-Resets the System during hangups due to power fluctuation

Heater Box

- Ceramic Infra Red Heater with higher power output and more durability than any tubular silicon quartz glass heaters
- Swivelling source box to take X-ray
- Temperature Resistant Design of heater box keeps exterior surface cool even after continuous use
- Stainless steel reflector and heater grill for complete cleaning of heater & reflector without any electrical shock hazards

LED Examination Lamp

Appropriate illumination to assess infant colour during procedures

Baby Bassinet (Stainless Steel)

- Easy access of an Infant from all sides due to clear acrylic collapsible side panels
- Acrylic Baby Tray for infant's head Up / Down facility
- Provision for positioning X-Ray cassette
- Thick cushion mattress
- Nylon based moulded side pillars to fix the drop down sides

Essential Attachments

Instrument Tray, Pole for Infusion Pump & IV Stand

Available Options

- Fabrication in Mild Steel or Stainless Steel
- Air/Pre-warm, Skin/Manual or Skin/Air/Manual (LCD) Controller

Temperature Controllers

Skin / Air / Manual (LCD)

Display

- 1" bright skin temp. display
- 1" bright air temp. display
- Numeric % of heater output display
- Set temp. display on LCD
- Control mode display on LCD
- APGAR Timer display on LCD

Manual Mode

- Time programmable
- Heater output adjustable
- Over temp. cutoff.
- Timer / APGAR Timer
- Baby attending alarm
- Mute time programmable
- Audio Alarm mute facility

Auto Mode

Safety alarm messages on LCD

Skin Mode

- "Skin Temp. High" ($>0.5^{\circ}\text{C}$ of set temp.)
- "Skin Temp. Low" ($<0.5^{\circ}\text{C}$ of set temp.)
- "Skin Temp. Over Range" ($>38^{\circ}\text{C}$)
- "Skin Temp. Under Range" ($<34^{\circ}\text{C}$)
- "Skin Probe Fail"

Air Mode

- "Air Temp. High" ($>1.5^{\circ}\text{C}$ of set temp.)
- "Air Temp. Low" ($<3.0^{\circ}\text{C}$ of set temp.)
- "Air Temp. Over Range" ($>39^{\circ}\text{C}$)
- "Air Probe Fail"

Safety high temp. cutoff at

- Skin temp. $>38^{\circ}\text{C}$
- Air temp. $>39^{\circ}\text{C}$
- Power Fail
- Heater Fail (optional)

Skin / Manual

Display

- 1" bright skin temp. display
- Set temp. display
- Numeric % of heater output display
- Selection of Skin & Manual modes

Manual Mode

- Time programmable
- Heater output adjustable
- Over temp. cutoff.
- Timer / APGAR Timer
- Baby attending alarm
- Mute time programmable
- Audio Alarm mute facility


Skin Mode

Safety alarm messages on LCD

- "Temp. High" ($<0.5^{\circ}\text{C}$ of set temp.)
- "Temp. Low" ($>0.5^{\circ}\text{C}$ of set temp.)
- "Temp. Over Range" ($>38^{\circ}\text{C}$) /
- "Temp. Under Range" ($<34^{\circ}\text{C}$)
- (Actual temp. starts blinking)
- "Probe Fail"
- Power failure

Safety high temp. cutoff at 38°C

For air control low temp. limit ($<34^{\circ}\text{C}$) can be programmed.



Bird Meditech

ISO 13485:2012 CERTIFIED COMPANY

www.birdmeditech.com

Available at:

XAVIER MED PVT. LTD.

1-10-51/2, Road 6B, Dwarakapuram,
Dilsukhnagar, Hyderabad - 500060

www.buyxavier.com

Customer Care: 8008895680

Service: 8008895079